




EG2001 Re-accurization (Accuracy Calibration)

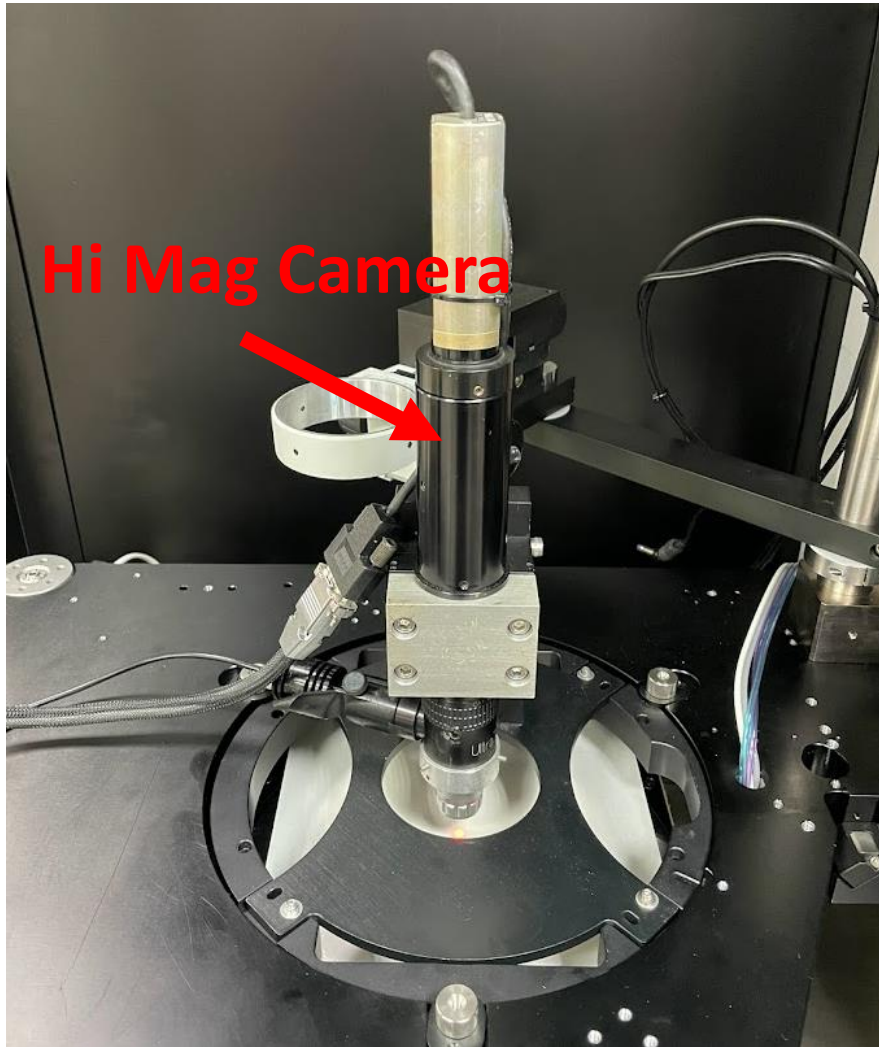


Total 7 Chips
Correction Prom will be create

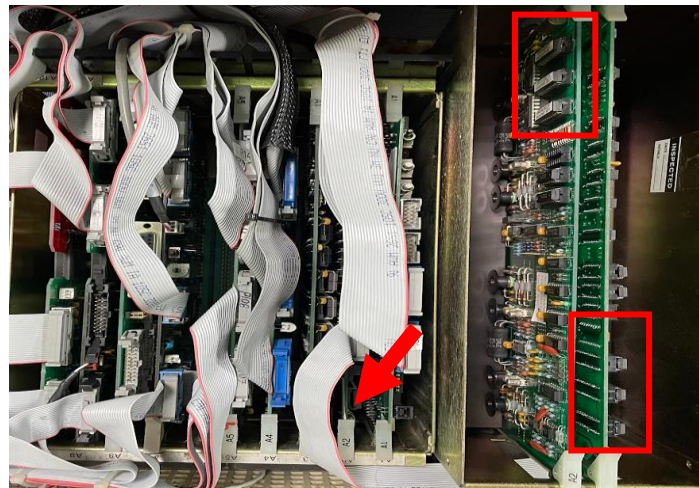

Probe Step Accuracy

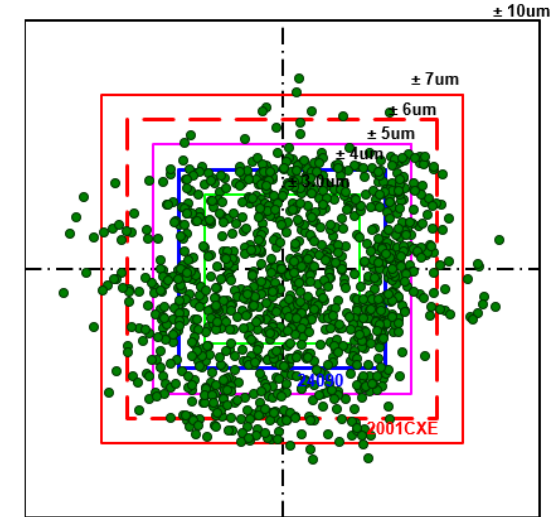

Before

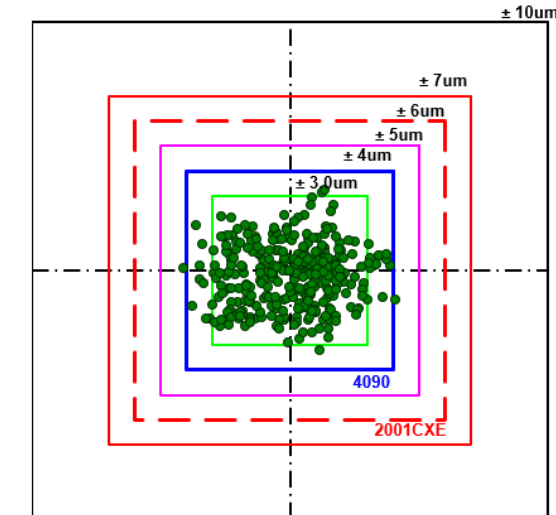

After

- *Re-accurization can only be done on original EG Forcer/Platen.
- *The Prober will meet EG SPEC within 0.5mil after re-accurization.
- *Dar board requirement: POWER DAR2 High Resolution